

PTS Panels™ Creatinine Test Strips

Distributed by

CLIAwaived™ Inc.



The PTS Panels Creatinine Test Strips are intended to measure Creatinine in whole blood. Creatinine measurements are used in the diagnosis and treatment of renal (kidney) diseases and in the monitoring of renal dialysis. This test is designed for use by healthcare professionals only with the CardioChek P•A Analyzer. A MEMo Chip is provided with each package of test strips and must be properly inserted into the analyzer before any test can be run. After the test strip is insert into the analyzer and blood applied to the strip, test results are displayed within 8 minutes. *For Professional Use Only.*

BENEFITS:

- Range: 0.2-10 mg/dL (17.8-885 mmol/L)
- Sample 20 µL whole blood (fingerstick or venous)
- Portable, easy-to-use
- Accurate results in minutes
- CLIA: Moderate Complexity (NOT CLIA Waived)
- FDA-Cleared


| Ordering Information: | |
|---|-----------------------|
| Product Description | Catalog # |
| PTS Panels™ Creatinine Test Strips (25 tests) | PTS-1720 |
| Reimbursement Information: | |
| CPT Code # | National Limit Amount |
| 82565 – Creatinine, blood | \$7.22 |

DISCLAIMER – The CPT information contained in this document is provided as representative examples of reimbursement in this category. It is intended to assist providers in accurately obtaining reimbursement for health care services. It is not intended to increase or maximize reimbursement by any payor. Providers should consult their payor organizations with regard to local reimbursement policies. The information provided in this document is for information purposes only and represents no statement, promise or guarantee by CLIAwaived™ Inc. All CPT codes are supplied for information purposes only and represent no statement; promise or guarantee by CLIAwaived™ Inc. that these codes will be appropriate or that reimbursement will be made. CPT codes and descriptions are copyrights of the American Medical Associations. CPT does not include fee schedules, relative values or related ratings. The source for this information is the Center for Medicare and Medicaid Services. The content provided by the Center for Medicare and Medicaid Services is updated frequently. It is the responsibility of the service provider to confirm the appropriate coding required by their local Medicare carriers, fiscal intermediaries and commercial payors. All product information and prices are subject to change without notice at any time. Please call our office before ordering to verify current prices.

PTS Panels™ Creatinine Strips Test Instructions

Be sure to read all instructions carefully before testing.

1. Insert the MEMo Chip that matches the lot number on the Test Strip vial and press one of the buttons to turn the analyzer ON.
2. Hold the Test Strip by the end with the horizontal raised lines. Insert the opposite end of the strip into analyzer. Push the strip in as far as it will go.

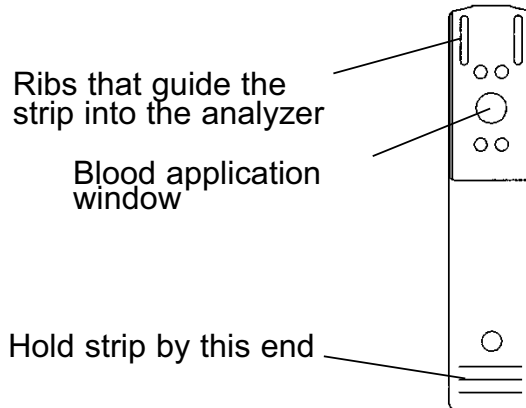

3. When APPLY SAMPLE appears on the display, use a capillary blood collector or pipet to apply 20 μ L of whole blood to the Test Strip blood application window.
4. Within eight minutes, the Creatinine result will appear on the display. Remove and discard strip. **DO NOT** add more blood to a Test Strip that has been used.

