

# FENTANYL/XYLAZINE RESIDUE TEST STRIP

A rapid, screening test for the qualitative detection of Fentanyl or Xylazine residue (e.g. dried liquid or powder) on surfaces, including the outer surface of pills.

**\*For Forensic Use only.**



## Features & Benefits

- Simple collection and testing procedure
  - Easy visual interpretation
  - Time to results: 3-10 minutes.
- Do not interpret results after 1 hour

The Fentanyl or Xylazine test strips are competitive binding lateral flow immunochromatographic assays for the qualitative detection of Fentanyl (FEN) or Xylazine (XYL) residue on surfaces, including the outer surface of pills.

### Test Procedure - Strip

- 1 Insert the extraction tube into the workstation and tear off the sealing film.
- 2 Insert a swab into the extraction tube for 5-20 seconds to wet it.
- 3 Use the wet swab to wipe across the surface several times to ensure adequate specimen is collected.
- 4 Insert the swab back into the extraction tube.
- 5 Roll the swab at least 5-10 times.
- 6 Press the head against the bottom and side of the extraction tube 10-20 times.
- 7 Insert the tip of the test strip into the extraction buffer, making sure the liquid is below the MAX line marked on the strip. Read the result at 3-10 minutes.

Positive      Negative      Invalid

## Ordering information

Product Description	Catalog No.	Format	Cut-off (ng/mL)	Kit Size
Fentanyl Residue Test Kit	GBFEN-1001a	Strip	5	20 Tests/Kit
Xylazine Residue Test Kit	GBXYL-1001a	Strip	50	20 Tests/Kit

# FENTANYL/XYLAZINE RESIDUE TEST CASSETTE

A rapid, screening qualitative test for the combo detection of fentanyl and Xylazine or for the single detection of fentanyl or Xylazine residue (e.g. dried liquid or powder) on surfaces, including the outer surface of pills.

For Forensic Use only.



Cassette


## Features & Benefits

- Simple collection and testing procedure
  - Easy visual interpretation
  - Time to results: 5-10 minutes.
- Do not interpret results after 1 hour

The Fentanyl/Xylazine, Fentanyl, or Xylazine tests are competitive binding lateral flow immunochromatographic assays for the qualitative detection of Fentanyl (FEN) and Xylazine (XYL) residue on surfaces, including the outer surface of pills, at the following cutoff concentrations

Test	Calibrator	Cut-off (ng/mL)
Fentanyl (FEN)	Fentanyl	5
Xylazine (XYL)	Xylazine	50

## Test Procedure - Cassette

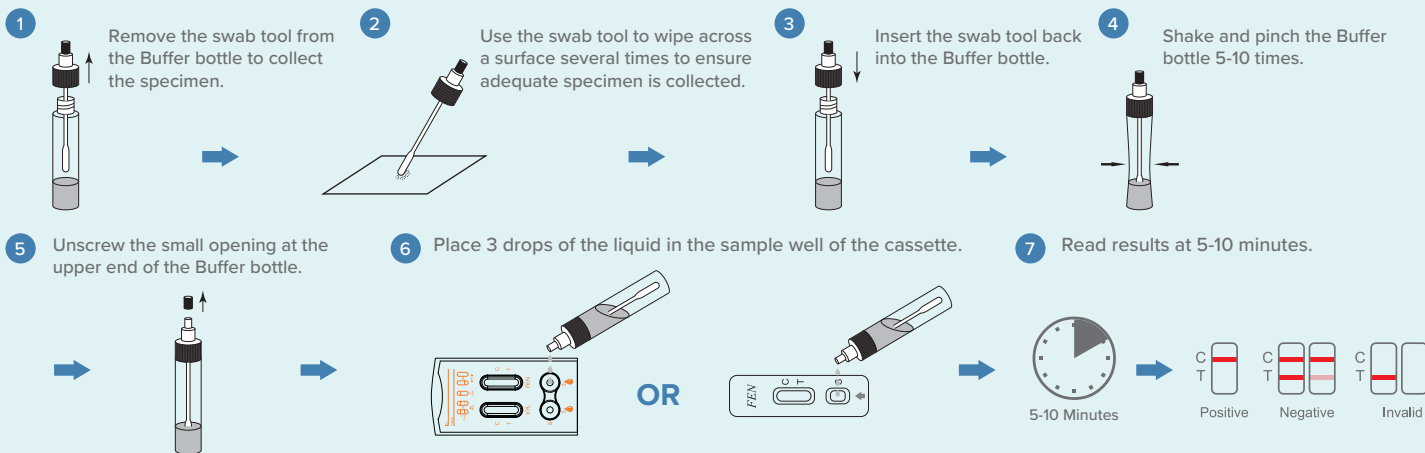

## Ordering information

Product Description	Format	Catalog No.	Kit Size
Fentanyl Residue Test Kit	Cassette	GBFEN-1002a	20 Tests/Kit
Xylazine Residue Test Kit	Cassette	GBXYL-1002a	20 Tests/Kit
Fentanyl/Xylazine Residue Test Kit	Cassette	GBDOA-1025-001	20 Tests/Kit